



| | |
|--------------|---|
| Title | Orthodontic aligner incorporating Eucommia ulmoides exerts low continuous force: In vitro study |
| Author(s) | Inoue, Sayuri; Yamaguchi, Satoshi; Uyama, Hiroshi et al. |
| Citation | Materials. 2020, 13(18), p. 4085 |
| Version Type | VoR |
| URL | https://hdl.handle.net/11094/93099 |
| rights | This article is licensed under a Creative Commons Attribution 4.0 International License. |
| Note | |

The University of Osaka Institutional Knowledge Archive : OUKA

<https://ir.library.osaka-u.ac.jp/>

The University of Osaka

Article

Orthodontic Aligner Incorporating *Eucommia ulmoides* Exerts Low Continuous Force: In Vitro Study

Sayuri Inoue ^{1,2}, Satoshi Yamaguchi ^{1,*} , Hiroshi Uyama ³ , Takashi Yamashiro ² and Satoshi Imazato ¹

¹ Department of Biomaterials Science, Osaka University Graduate School of Dentistry, 1-8 Yamadaoka, Suita, Osaka 565-0871, Japan; sayuri-inoue@dent.osaka-u.ac.jp (S.I.); imazato@dent.osaka-u.ac.jp (S.I.)

² Department of Orthodontics and Dentofacial Orthopedics, Osaka University Graduate School of Dentistry, 1-8 Yamadaoka, Suita, Osaka 565-0871, Japan; yamashiro@dent.osaka-u.ac.jp

³ Division of Applied Chemistry, Osaka University Graduate School of Engineering, 2-1 Yamadaoka, Suita, Osaka 565-0871, Japan; uyama@chem.eng.osaka-u.ac.jp

* Correspondence: yamagu@dent.osaka-u.ac.jp; Tel.: +81-6-6879-2917

Received: 4 August 2020; Accepted: 11 September 2020; Published: 14 September 2020



Abstract: The aim of this study was to investigate the orthodontic force exerted by thermoplastic orthodontic appliances incorporating *Eucommia ulmoides* in terms of usefulness as the aligner-type orthodontic device. Erkodur, Essix C+[®], *Eucommia* elastomer, and edgewise brackets were used ($n = 3$, each; thickness = 1.0 mm, each). The orthodontic force on the upper right incisor was measured every 24 h for two weeks using a custom-made measuring device. The force of the *Eucommia* elastomer (4.25 ± 0.274 N) and multi bracket system (5.32 ± 0.338 N) did not change from the beginning to the end ($p > 0.01$). The orthodontic force exerted by the *Eucommia* elastomer was lower than that of the multi-bracket orthodontic appliance from the beginning to the end. The force of Erkodur significantly decreased from the beginning to 24 h (6.47 ± 1.40 N) and 48 h (3.30 ± 0.536 N) ($p < 0.01$). The force of Essix C+[®] significantly decreased from the beginning (13.2 ± 0.845 N) to 24 h (8.77 ± 0.231 N) ($p < 0.01$). The thermoplastic orthodontic appliance made of *Eucommia* elastomer continuously exerted a constant orthodontic force for two weeks under water immersion conditions. The orthodontic force of *Eucommia* elastomer was found to be similar to the orthodontic force exerted by the multi-bracket orthodontic appliance with 0.019×0.025 in nickel–titanium wire. These results suggest that the *Eucommia* elastomer has possibly become one of the more useful materials to form thermoplastic orthodontic appliance exerting low continuous orthodontic force.

Keywords: orthodontic appliance; thermoplastics; *Eucommia ulmoides*; orthodontic wires

1. Introduction

Orthodontic treatment using a transparent thermoplastic orthodontic appliance, called aligner-type orthodontic devices, has recently increased with the aesthetic demands of patients. Aligner-type orthodontic devices appeared in the early 1970s as a retainer for preventing relapse of the teeth after orthodontic treatment [1], then they started to be used for minor tooth movement [2]. To date, it has been devised in a variety of materials and thicknesses for efficient orthodontic treatment [3–5]. At present, the method for fabricating an aligner using a digital setup model designed by simulating tooth movement via a computer has become widespread, and orthodontic treatment by aligner has expanded the range of application from minor tooth movement to whole teeth orthodontic treatment to full jaw treatment [6–9]. With the spread of orthodontic treatment using thermoplastic orthodontic appliances, many experiments have been conducted to investigate the orthodontic force exerted by such

appliances. At present, the most thermoplastic materials used for aligners are made by polyethylene terephthalate glycol (PETG), but there are other materials made of polyurethane (PU) or polyethylene terephthalate (PET) [4,10]. Furthermore, new thermoplastic materials have also been developed such as by mixing PETG, PU, and polycarbonate at unique blending ratios [4] and by using PU with shape memory functions [11].

However, the amount of tooth movement using an aligner is limited to a range of 0.25 mm to 1.0 mm [3,12], so approximately 50 aligners may be required to complete orthodontic treatment. In addition, after setting an aligner on dentition, the teeth are subjected to an excessive orthodontic force, and then the force decreases over time. In the current treatment system, a new aligner must be replaced every 10 to 14 days.

Therefore, to make orthodontic treatment with an aligner more efficient, the development of a new thermoplastic materials that can continuously exert suitable orthodontic force for tooth movement are required.

Eucommia elastomer (EE), a trans-1,4-polyisoprene extracted and purified from *Eucommia ulmoides*, is a highly biosafety polymer exhibiting high tensile properties and large breaking strain [13]. As a tensile property, it shows high stress to initial strain, but after that it shows constant stress even if strain increases. Therefore, it can be expected that an aligner made from EE is suitable for tooth movement and be able to exert a constant orthodontic force. However, there have only been a few studies of the physical properties of the thermoplastic orthodontic materials [4,10,14–18] and the orthodontic force exerted by the aligner [19–23]. In this study, we focused on the high ductility of EE and aimed to evaluate an aligner-type orthodontic device that is suitable for the movement of teeth and that expresses weak and sustained orthodontic force.

The aim of this study was to investigate the orthodontic force exerted by thermoplastic orthodontic appliances incorporating *Eucommia ulmoides* in terms of usefulness as the aligner-type orthodontic device.

2. Materials and Methods

2.1. Specimen Preparation

Erkodur (ER) (ERKODENT Erich Kopp GmbH, Pfalzgrafenweiler, Germany), Essix C+® Plastic (EC) (DENTSPLY Raintree Essix, Sarasota, FL, USA), and (EE) (Hitachi Zosen, Osaka, Japan) were used. Trans-1,4-polyisoprene powder extracted and purified from *Eucommia ulmoides* was fused and was formed as EE by mold injection. All of these materials were 1.0 mm thick single-layer materials with 120.0 mm in diameter (Table 1).

Table 1. Orthodontic thermoplastic materials used in this study.

| Product | Code | Manufacturer | Composition |
|---------------------------|------|--------------------------|--|
| Erkodur | ER | Erkodent Erich Kopp GmbH | Polyethylene terephthalate glycol (PETG) |
| Essix C+® Plastic | EC | DENTSPLY Raintree Essix | Polypropylene (PP) |
| <i>Eucommia</i> elastomer | EE | Hitachi Zosen | <i>Eucommia ulmoides</i> |

The standard dental model (E50-500AU, NISSHIN, Kyoto, Japan) was duplicated using a 3D scanner (S-WAVE D900, SHOFU, Kyoto, Japan) and 3D printer (AGILISTA-3200, KEYENCE, Osaka, Japan) as the normal dentition. The aligners were formed using ER and EC according to the instructions of the manufacturer ($n = 3$, each). The ER was heated to 160 °C, pressed to the model, and cooled for 45 s using a vacuum-forming machine (Elkopress 300Tp, ERKODENT Erich Kopp GmbH, Germany) (Figure 1). The EC was heated to 220 °C for 50 s, pressed to the model and cooled for 120 s using a vacuum-forming machine (Biostar VII JM Ortho, Tokyo, Japan) (Figure 1). The EE was heated to 220 °C for 20 s, pressed to the model, and cooled for 240 s using the same vacuum-forming machine as EC (Figure 1).

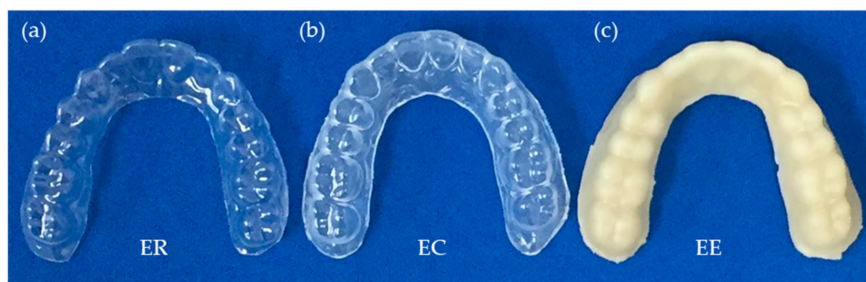


Figure 1. (a) Aligner formed using ER; (b) aligner formed using EC, and (c) aligner formed using EE.

2.2. Characterization of Eucommia Elastomer

Five round specimens ($\phi 15 \times 1.0$ mm) of EE was prepared and water absorption test was conducted according to ISO 4049:2019 [24] ($n = 5$). Test specimens were prepared similar to the water absorption test and subjected to X-ray diffraction (XRD) analysis (Rint2000, Rigaku, Tokyo, Japan) in dry condition. The XRD analysis was conducted at 2θ range between 2° and 60° with a step size of 0.02° in a continuous mode of $4.0^\circ/\text{min}$. Fourier transformation infrared spectroscopy (FTIR) was conducted. Part of each material ($6.0 \times 6.0 \times 1.0$ mm) was prepared and the spectra were recorded with an FTIR spectrometer (FT-IR 8300, Shimadzu, Kyoto, Japan) and averaged over 20 scans between $700\text{--}4000\text{ cm}^{-1}$. Ten specimens of 1.0 mm thickness were prepared according to ISO 527-2 type 5B [25]. Five specimens were immersed in distilled water at 37°C with no strain for 24 h and two weeks. The remaining specimens were loaded to 1% strain with the custom-made loading device developed in previous study [18] and were stored in distilled water at 37°C for two weeks. Tensile tests were conducted with a universal testing machine (EZ-SX, Shimadzu, Kyoto, Japan) with a 500 N load cell, and an elastic modulus was determined from the slope of the obtained stress–strain curve. Physical properties of ER and EC have been measured in a previous study [18] and compared to those of EE.

2.3. Evaluation of Orthodontic Force

Using 3D data of the standard model (E50-500AU, Nisshin, Kyoto, Japan), the stainless-steel-made dentition model was prepared where the upper right central incisor was tipped 3° labially (TRUESEED, Kyoto, Japan) as the crowded dentition. A force sensor (Nitta, Osaka, Japan) was attached to at the middle of root of the upper right central incisor (Figure 2a). Aligner-type orthodontic devices using thermoplastic materials were applied to the dentition model, and they were immersed to 37°C distilled water using a custom-made linear actuator (TRUESEED) (Figure 2b,c) to replicate the oral cavity conditions. Using the actuator, the orthodontic force on upper right incisor was measured every 24 h for two weeks.

2.4. Multi-Bracket Orthodontic Appliance Model

To compare the force, the orthodontic force exerted by multi-bracket orthodontic appliances using nickel titanium wire and metal brackets was measured using the same dentition model. The 0.022×0.028 inch slot brackets (VictoryTM, 3M Japan, Tokyo, Japan) were attached to the dentition model using light-cure orthodontic adhesive system (Beauty Ortho Bond II, SHOFU, Kyoto, Japan) and metal primer (METHAL PRIMER Z, GC, Tokyo, Japan). The 0.019×0.025 in nickel titanium wire (Naitenol classic archwire, 3M Japan, Tokyo, Japan) were prepared and inserted to the dentition model (Figure 3). They were also immersed 37°C distilled water for two weeks and the force were measured every 24 h.

2.5. Statistical Analysis

The mean amount of water absorption of EE after 24 h and two weeks were analyzed by the Student's *t*-test. The mean elastic modulus of EE after 24 h without strain and two weeks with 1% constant strain were analyzed by the Student's *t*-test. The *p*-values of less than 0.05 were considered as

statistically significant. The mean force in each group were statistically analyzed by one-way analysis of variance (ANOVA) and Dunnett's test (PASW Statistics 18, IBM, Somers, NY, USA). The p -values of less than 0.01 were considered as statistically significant.

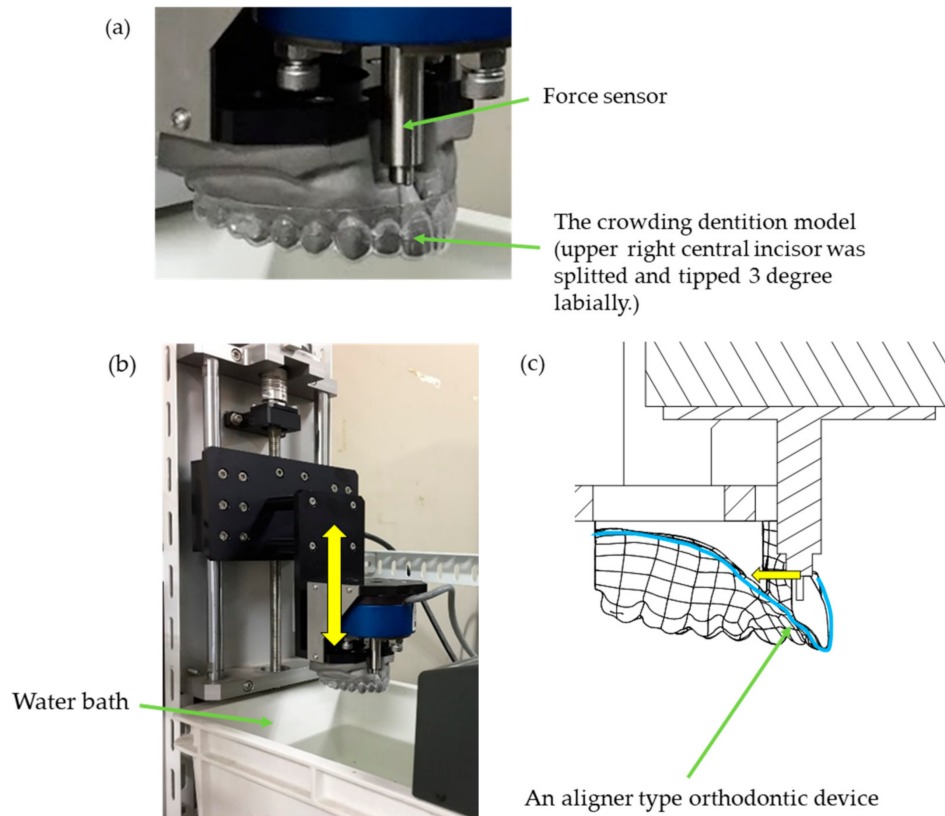


Figure 2. Custom-made device for measuring orthodontic force. (a) The upper right central incisor was tilted 3° to labially, a force sensor was installed at the root 1/2 position, and an ER or EC aligner was put on the model. (b) The model was fixed to a linear actuator and immersed in a constant temperature bath at 37°C by adjusting the height (yellow arrow in the figure). (c) The model and force sensor. The orthodontic force in the direction of the yellow arrow expressed by the aligner-type orthodontic device (light blue line) was measured at a cycle of 10 times/s.

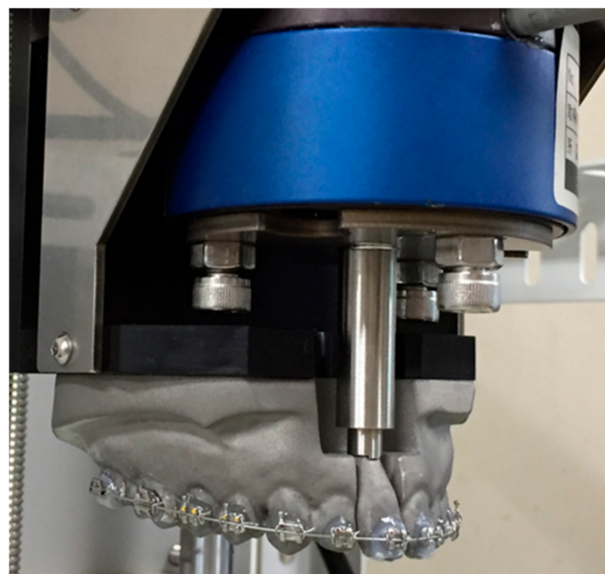


Figure 3. A multi-bracket orthodontic appliance model.

3. Results

The amount of water absorption of EE after 24 h and two weeks were $0.0344 \pm 0.4291 \mu\text{g}/\text{mm}^3$ and $0.8761 \pm 0.3730 \mu\text{g}/\text{mm}^3$, respectively, and a significant difference was found ($p < 0.05$). The XRD patterns of EE are shown in Figure 4. Diffraction patterns indicated that EE was a crystalline polymer same as EC [17]. The infrared absorption spectrum obtained by FTIR analysis of EE showed molecular structure based on covalent bond between carbon and hydrogen (Figure 5). The elastic modulus of EE when immersed in distilled water for 24 h without strain and two weeks with 1% constant strain were $137.4 \pm 6.867 \text{ MPa}$ and $131.8 \pm 11.09 \text{ MPa}$, respectively. There was no significant difference in both elastic moduli ($p > 0.05$).

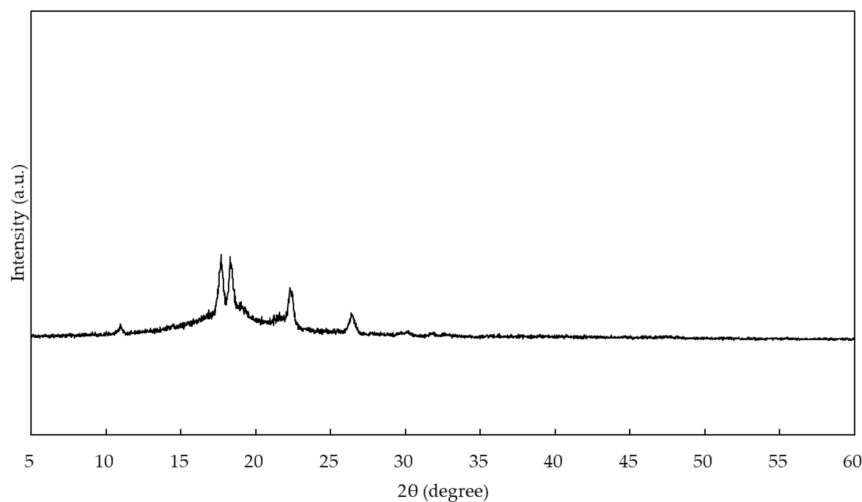


Figure 4. X-ray diffraction pattern of EE.

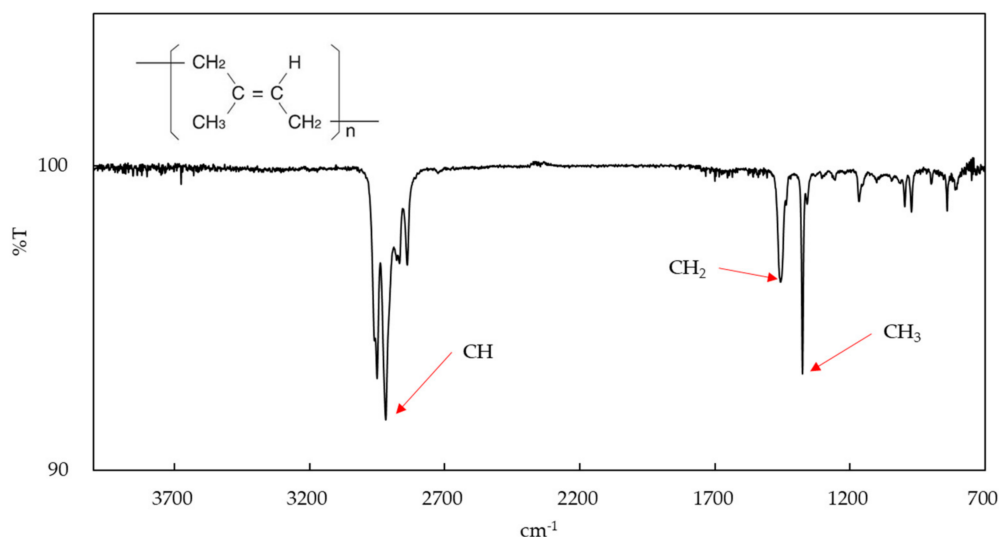


Figure 5. Infrared absorption spectrum for EE.

Figure 6 shows the force of each aligner-type orthodontic device and multi bracket system obtained by the custom-made orthodontic force measurement device. The force of EE ($4.25 \pm 0.274 \text{ N}$) and multi bracket system ($5.32 \pm 0.338 \text{ N}$) did not change from the beginning to the end ($p > 0.01$). The orthodontic force exerted by EE was lower than that of multi-bracket orthodontic appliance from the beginning to the end. The force of ER was significantly decreased from the beginning to 24 h ($6.47 \pm 1.40 \text{ N}$) and 48 h ($3.30 \pm 0.536 \text{ N}$) ($p < 0.01$). The force of EC was significantly decreased from the beginning ($13.2 \pm 0.845 \text{ N}$) to 24 h ($8.77 \pm 0.231 \text{ N}$) ($p < 0.01$).

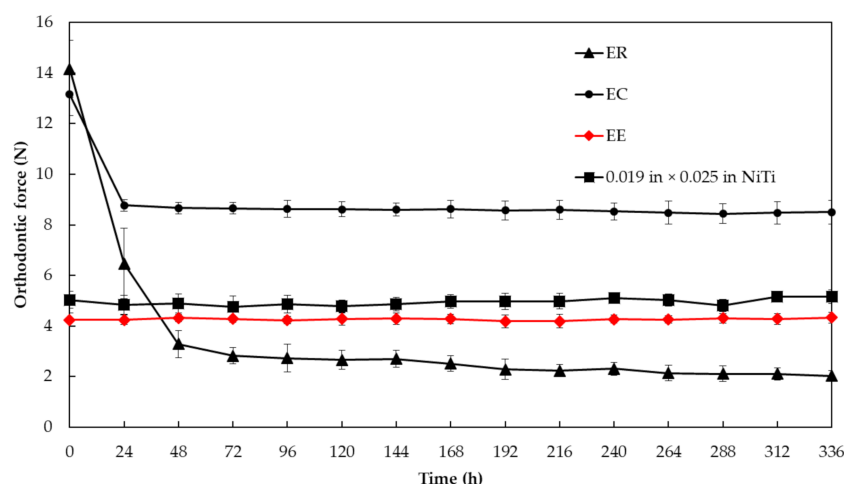


Figure 6. Orthodontic force measured from each material.

4. Discussion

Various measuring devices have been reported for orthodontic force [17,19,21–23]. In this study, an orthodontic force measurement device was designed which can measure the reaction force generated at the middle of root of the upper right central incisor using a force sensor, and the force was measured. Our measuring device is unique because there is no previous research that measured the force while immersing in water with the aligner attached to the dental arch. This experiment simulated the same dentition model also in the multi-bracket orthodontic appliance as the thermoplastic orthodontic appliance, it was possible to directly compare it with the force exerted by EE aligner. In addition, by measuring the force for two weeks, it was possible to clarify the change of the force exerted by the thermoplastic orthodontic appliances. In ER and EC, the force in the first 24 to 48 h significantly decreased. Li et al. [19] measured the force over the time for two weeks when an aligner made of 1.0 mm thick ER was attached to a dental model twice the size in which the upper right central incisor was inclined to labial side. It was reported that a significant decrease force was observed in the first eight hours [19]. Fang et al. [14] reported that a stress relaxation test was conducted by applying 5% constant strain to a dumbbell-shaped specimen of ER, and that stress relaxation was promoted under water immersion condition. The results of our study showing that the force of ER decreased early in the period are consistent with these reports.

The EE demonstrated a lower amount of water absorption than both ER and EC [18]. Also, the EE was a crystalline polymer tending to low water absorption such as EC [18]. Even when immersed in distilled water for two weeks with constant strain, the elastic modulus of EE was not varied and lower than those of ER and EC [18]. The EE aligner used in this experiment did not change its force for two weeks after the start of the measurement and exhibited similar properties as the nickel titanium wire. These results suggest that an aligner made from EE may be able to continue tooth movement for more than two weeks, and it is expected that the replacement period can be set to two weeks or more, unlike the existing system.

In ER, it has been reported that the force that exerts as tooth displacement increases also increases [19,21,22]. On the other hand, the EE has high ductility, so even if the displacement amount increases, the force that is developed does not increase, and it may be possible to set the movement amount of teeth with one device large.

The optimal correction force for multi-bracket devices is said to be in the range of 0.343 to 0.980 N [26] or not exceed 0.588 N [27]. The force of EE and nickel–titanium wire obtained by our research was higher than those. Barbagallo [20] measured force when the maxillary first premolar tipped buccal side by 0.5 mm using an aligner made of ER with a thickness of 0.8 mm for patients with moderate crowding using a film sheet capable of measuring the pressure [20]. The orthodontic force that

was initially developed was 5.12 N, and 1.2 N after two weeks of wear. These forces were also greater than the force suggested by Proffit et al. [26] and Reitan [27] above. That is, even if movement of the teeth and buffering of the force by other factors, such as the periodontal ligament and the alveolar bone occur in the body, the initial force developed by the aligner is basically larger than the nickel–titanium wire. Excessive force can contribute to root resorption that occurs during orthodontic treatment [28].

Schwarz [29] has reports that when a load of more than 0.255 N per unit area is applied to the root, an anemia is formed in the periodontal ligament and the root is absorbed. Based on Jepsen's [30] report that the root surface area of the first premolar is $2.34 \pm 0.33 \text{ cm}^2$ [30], it can be calculated that root resorption occurs in the first premolar when it exceeds 0.681 N, but the value indicated by Barbagallo [20] exceeded the force. On the other hand, Gay et al. [31] and Iglesias-Linares et al. [32] reported that the frequency of root resorption in patients treated with aligner-type orthodontic devices made from PU was not significantly different from that using multi-bracket devices. A variety of factors are involved in root resorption such as patient's gene characteristics [33], dynamic length of orthodontic treatment [34], tooth movement direction [35,36]. For this reason, it is difficult to evaluate its usefulness based on the orthodontic force alone, but it will be necessary to further study.

In addition, the thermoplastic materials' wear, perforation, and cracking of the aligner has been reported as an issue [37,38], and the deposition of calcium phosphate [39] was induced when using an aligner. In the future, further verification experiments will be required for clinical application of EE including wear tests.

Furthermore, the EE is made from a natural plant and biocompatibility was confirmed according to ISO 10993 [40,41]; it is eco-friendly compared to conventional thermoplastic orthodontic materials. As the main limitation of this study, the EE aligner is yellowish due to the fact of its original color of the plant as shown in Figure 1c and thus improvements to make it white or transparent are necessary when considering clinical application. Moreover, the EE has a weak to high temperature and paying attention to the heat for molding was required.

5. Conclusions

The thermoplastic orthodontic appliances incorporating *Eucommia ulmoides* continuously exerted a constant orthodontic force for two weeks under water immersion conditions. The orthodontic force of *Eucommia* elastomer was found to be similar to the orthodontic force exerted by the multi-bracket orthodontic appliance with 0.019×0.025 in nickel–titanium wire. Those results suggest that the *Eucommia* elastomer is possibly become one of useful materials to form thermoplastic orthodontic appliance exerting low continuous orthodontic force.

Author Contributions: Conceptualization, T.Y. and S.I. (Satoshi Imazato); methodology, S.I. (Sayuri Inoue) and S.Y.; validation, S.I. (Sayuri Inoue) and S.Y.; formal analysis, S.I. (Sayuri Inoue); investigation, S.I. (Sayuri Inoue) and S.Y.; resources, H.U.; data curation, S.I. (Sayuri Inoue); writing—original draft preparation, S.I. (Sayuri Inoue); writing—review and editing, S.Y. and S.I. (Satoshi Imazato); visualization, S.I. (Sayuri Inoue) and S.Y.; supervision, S.Y.; project administration, T.Y. and S.I. (Satoshi Imazato). All authors have read and agreed to the published version of the manuscript.

Funding: This research received no external funding.

Acknowledgments: We appreciate for the synthesis of *Eucommia* elastomer by Hitachi Zosen.

Conflicts of Interest: The authors declare no conflict of interest.

References

1. Ponitz, R.J. Invisible retainers. *Am. J. Orthod.* **1971**, *59*, 266–272. [[CrossRef](#)]
2. A McNamara, J.; Kramer, K.L.; Juenker, J.P. Invisible retainers. *J. Clin. Orthod. JCO* **1985**, *19*, 570–578. [[PubMed](#)]
3. Sheridan, J.J. The Essix bracket choice appliance. *J. Clin. Orthod. JCO* **1996**, *30*, 203–205. [[PubMed](#)]
4. Zhang, N.; Bai, Y.; Ding, X.; Zhang, Y. Preparation and characterization of thermoplastic materials for invisible orthodontics. *Dent. Mater. J.* **2011**, *30*, 954–959. [[CrossRef](#)]
5. Sanchez, J.F.; Ramirez, I.P.; Alonso, J.M. Osamu active retainer for correction of mild relapse. *J. Clin. Orthod. JCO* **1998**, *32*, 26–28.

6. Zawawi, K.H. Orthodontic Treatment of a Mandibular Incisor Extraction Case with Invisalign. *Case Rep. Dent.* **2014**, *2014*, 1–4. [[CrossRef](#)]
7. Frongia, G.; Castroflorio, T. Correction of severe tooth rotations using clear aligners: A case report. *Aust. Orthod. J.* **2012**, *28*, 245–249.
8. Schupp, W.; Haubrich, J.; Neumann, I. Treatment of anterior open bite with the Invisalign system. *J. Clin. Orthod. JCO* **2010**, *44*, 501–507.
9. Giancotti, A.; Mampieri, G.; Greco, M. Correction of deep bite in adults using the Invisalign system. *J. Clin. Orthod. JCO* **2008**, *42*, 719–726.
10. Lombardo, L.; Martines, E.; Mazzanti, V.; Arreghini, A.; Mollica, F.; Siciliani, G. Stress relaxation properties of four orthodontic aligner materials: A 24-hour in vitro study. *Angle Orthod.* **2017**, *87*, 11–18. [[CrossRef](#)]
11. Sokolowski, W.; Metcalfe, A.; Hayashi, S.; Yahia, L.; Raymond, J. Medical applications of shape memory polymers. *Biomed. Mater.* **2007**, *2*, S23–S27. [[CrossRef](#)] [[PubMed](#)]
12. Kim, T.-W.; Echarri, P. Clear aligner: An efficient, esthetic, and comfortable option for an adult patient. *World J. Orthod.* **2007**, *8*, 13–18.
13. Nakazawa, Y.; Takeda, T.; Suzuki, N.; Hayashi, T.; Harada, Y.; Bamba, T.; Kobayashi, A. Histochemical study of trans-polyisoprene accumulation by spectral confocal laser scanning microscopy and a specific dye showing fluorescence solvatochromism in the rubber-producing plant, *Eucommia ulmoides* Oliver. *Planta* **2013**, *238*, 549–560. [[CrossRef](#)] [[PubMed](#)]
14. Fang, D.; Zhang, N.; Chen, H.; Bai, Y. Dynamic stress relaxation of orthodontic thermoplastic materials in a simulated oral environment. *Dent. Mater. J.* **2013**, *32*, 946–951. [[CrossRef](#)] [[PubMed](#)]
15. Ryokawa, H.; Miyazaki, Y.; Fujishima, A.; Miyazaki, T.; Maki, K. The mechanical properties of dental thermoplastic materials in a simulated intraoral environment. *Orthod. Waves* **2006**, *65*, 64–72. [[CrossRef](#)]
16. Kwon, J.-S.; Lee, Y.-K.; Lim, B.-S.; Lim, Y.-K. Force delivery properties of thermoplastic orthodontic materials. *Am. J. Orthod. Dentofac. Orthop.* **2008**, *133*, 228–234. [[CrossRef](#)]
17. Iijima, M.; Kohda, N.; Kawaguchi, K.; Muguruma, T.; Ohta, M.; Naganishi, A.; Murakami, T.; Mizoguchi, I. Effects of temperature changes and stress loading on the mechanical and shape memory properties of thermoplastic materials with different glass transition behaviours and crystal structures. *Eur. J. Orthod.* **2015**, *37*, 665–670. [[CrossRef](#)]
18. Inoue, S.; Yamaguchi, S.; Uyama, H.; Yamashiro, T.; Imazato, S. Influence of constant strain on the elasticity of thermoplastic orthodontic materials. *Dent. Mater. J.* **2020**, *39*, 415–421. [[CrossRef](#)]
19. Li, X.; Ren, C.; Wang, Z.; Zhao, P.; Wang, H.; Bai, Y. Changes in force associated with the amount of aligner activation and lingual bodily movement of the maxillary central incisor. *Korean J. Orthod.* **2016**, *46*, 65–72. [[CrossRef](#)]
20. Barbagallo, L.J.; Shen, G.; Jones, A.S.; Swain, M.; Petocz, P.; Darendeliler, M.A. A Novel Pressure Film Approach for Determining the Force Imparted by Clear Removable Thermoplastic Appliances. *Ann. Biomed. Eng.* **2007**, *36*, 335–341. [[CrossRef](#)]
21. Hahn, W.; Fialka-Fricke, J.; Dathe, H.; Fricke-Zech, S.; Zapf, A.; Gruber, R.; Kubein-Meesenburg, D.; Sadat-Khonsari, R. Initial forces generated by three types of thermoplastic appliances on an upper central incisor during tipping. *Eur. J. Orthod.* **2009**, *31*, 625–631. [[CrossRef](#)] [[PubMed](#)]
22. Elkholy, F.; Panchaphongsaphak, T.; Kilic, F.; Schmidt, F.; Lapatki, B. Forces and moments delivered by PET-G aligners to an upper central incisor for labial and palatal translation. *J. Orofac. Orthop./Fortschr. Kieferorthop.* **2015**, *76*, 460–475. [[CrossRef](#)] [[PubMed](#)]
23. Kohda, N.; Iijima, M.; Muguruma, T.; A Brantley, W.; Ahluwalia, K.S.; Mizoguchi, I. Effects of mechanical properties of thermoplastic materials on the initial force of thermoplastic appliances. *Angle Orthod.* **2012**, *83*, 476–483. [[CrossRef](#)]
24. Dentistry. Polymer-based restorative materials. *BSI Br. Stand* **2013**. [[CrossRef](#)]
25. ISO527-2:2012. *Plastics—Determination of Tensile Properties—Part 2: Test Conditions for Moulding and Extrusion Plastics*; International Organization for Standardization: Chiswick, London, UK, 2012.
26. Proffit, W.R.; Fields, H.W.; Sarver, D.M. *Contemporary Orthodontics*, 4th ed.; Mosby Elsevier: St. Louis, MO, USA, 2007.
27. Reitan, K. Clinical and histologic observations on tooth movement during and after orthodontic treatment. *Am. J. Orthod.* **1967**, *53*, 721–745. [[CrossRef](#)]

28. Chan, E.; Darendeliler, M.A. Physical properties of root cementum: Part 7. Extent of root resorption under areas of compression and tension. *Am. J. Orthod. Dentofac. Orthop.* **2006**, *129*, 504–510. [\[CrossRef\]](#)
29. Schwarz, A.M. Tissue changes incidental to orthodontic tooth movement. *Int. J. Orthod. Oral Surg. Radiogr.* **1932**, *18*, 331–352. [\[CrossRef\]](#)
30. Jepsen, A. Root Surface Measurement and A Method for X-Ray Determination of Root Surface Area. *Acta Odontol. Scand.* **1963**, *21*, 35–46. [\[CrossRef\]](#)
31. Gay, G.; Ravera, S.; Castroflorio, T.; Garino, F.; Rossini, G.; Parrini, S.; Cugliari, G.; Deregibus, A.P. Root resorption during orthodontic treatment with Invisalign®: A radiometric study. *Prog. Orthod.* **2017**, *18*, 12. [\[CrossRef\]](#)
32. Iglesias-Linares, A.; Sonnenberg, B.; Solano, B.; Yañez-Vico, R.-M.; Solano, E.; Lindauer, S.J.; Flores-Mir, C. Orthodontically induced external apical root resorption in patients treated with fixed appliances vs removable aligners. *Angle Orthod.* **2017**, *87*, 3–10. [\[CrossRef\]](#)
33. Al-Qawasmi, R.; Hartsfield, J.; Everett, E.; Flury, L.; Liu, L.; Foroud, T.; Macri, J.; Roberts, W. Genetic predisposition to external apical root resorption in orthodontic patients: Linkage of chromosome-18 marker. *J. Dent. Res.* **2003**, *82*, 356–360. [\[CrossRef\]](#) [\[PubMed\]](#)
34. Brin, I.; Tulloch, J.; Koroluk, L.; Philips, C. External apical root resorption in Class II malocclusion: A retrospective review of 1- versus 2-phase treatment. *Am. J. Orthod. Dentofac. Orthop.* **2003**, *124*, 151–156. [\[CrossRef\]](#)
35. Han, G.; Huang, S.; Hoff, J.W.V.D.; Zeng, X.; Kuijpers-Jagtman, A.M. Root resorption after orthodontic intrusion and extrusion: An intraindividual study. *Angle Orthod.* **2005**, *75*, 912–918. [\[PubMed\]](#)
36. Harris, D.A.; Jones, A.S.; Darendeliler, M.A. Physical properties of root cementum: Part 8. Volumetric analysis of root resorption craters after application of controlled intrusive light and heavy orthodontic forces: A microcomputed tomography scan study. *Am. J. Orthod. Dentofac. Orthop.* **2006**, *130*, 639–647. [\[CrossRef\]](#) [\[PubMed\]](#)
37. Raja, T.A.; Littlewood, S.J.; Munyombwe, T.; Bubb, N.L. Wear resistance of four types of vacuum-formed retainer materials: A laboratory study. *Angle Orthod.* **2014**, *84*, 656–664. [\[CrossRef\]](#) [\[PubMed\]](#)
38. Gardner, G.D.; Dunn, W.J.; Taloumis, L. Wear comparison of thermoplastic materials used for orthodontic retainers. *Am. J. Orthod. Dentofac. Orthop.* **2003**, *124*, 294–297. [\[CrossRef\]](#)
39. Eliades, T.; Bourauel, C. Intraoral aging of orthodontic materials: The picture we miss and its clinical relevance. *Am. J. Orthod. Dentofac. Orthop.* **2005**, *127*, 403–412. [\[CrossRef\]](#)
40. ISO 10993-5:2009. *Biological Evaluation of Medical Devices—Part 5: Tests for In Vitro Cytotoxicity*; International Organization for Standardization: Chiswick, London, UK, 2009.
41. ISO 10993-10:2010. *Biological Evaluation of Medical Devices—Part 10: Tests for Irritation and Skin Sensitization*; International Organization for Standardization: Chiswick, London, UK, 2010.

