




Title	A case report of pre-implantation feasibility test for combining leadless pacemaker and subcutaneous implantable cardioverter-defibrillator in adult congenital heart disease
Author(s)	Mima, Hibiki; Oka, Takafumi; Sera, Fusako et al.
Citation	Journal of Cardiology Cases. 2024, 30(6), p. 189–192
Version Type	AM
URL	<a href="https://hdl.handle.net/11094/98239">https://hdl.handle.net/11094/98239</a>
rights	© 2024. This manuscript version is made available under the CC-BY-NC-ND 4.0 license <a href="https://creativecommons.org/licenses/by-nc-nd/4.0/">https://creativecommons.org/licenses/by-nc-nd/4.0/</a>
Note	

*The University of Osaka Institutional Knowledge Archive : OUKA*


<https://ir.library.osaka-u.ac.jp/>

The University of Osaka

A

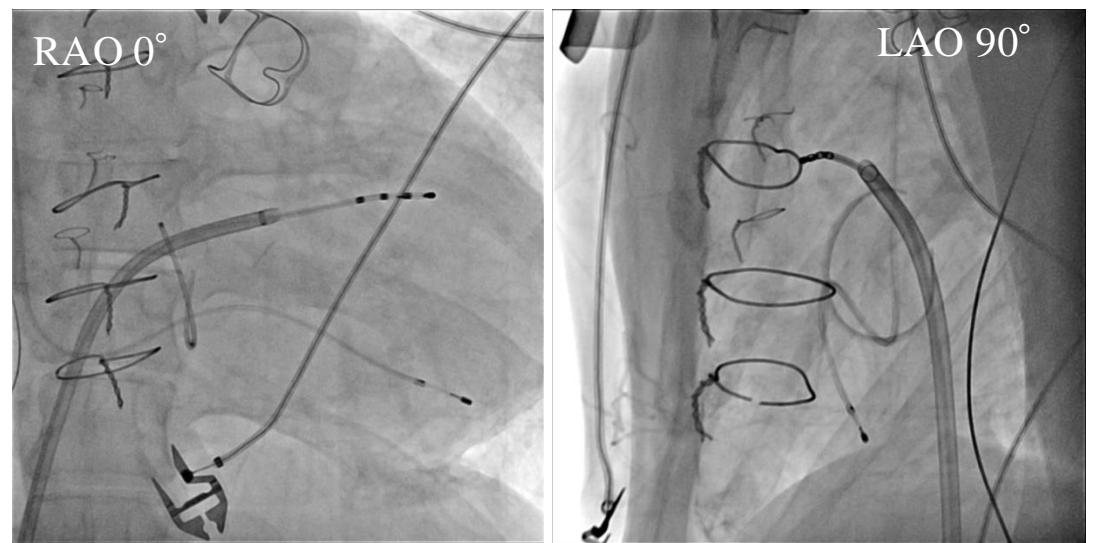

B

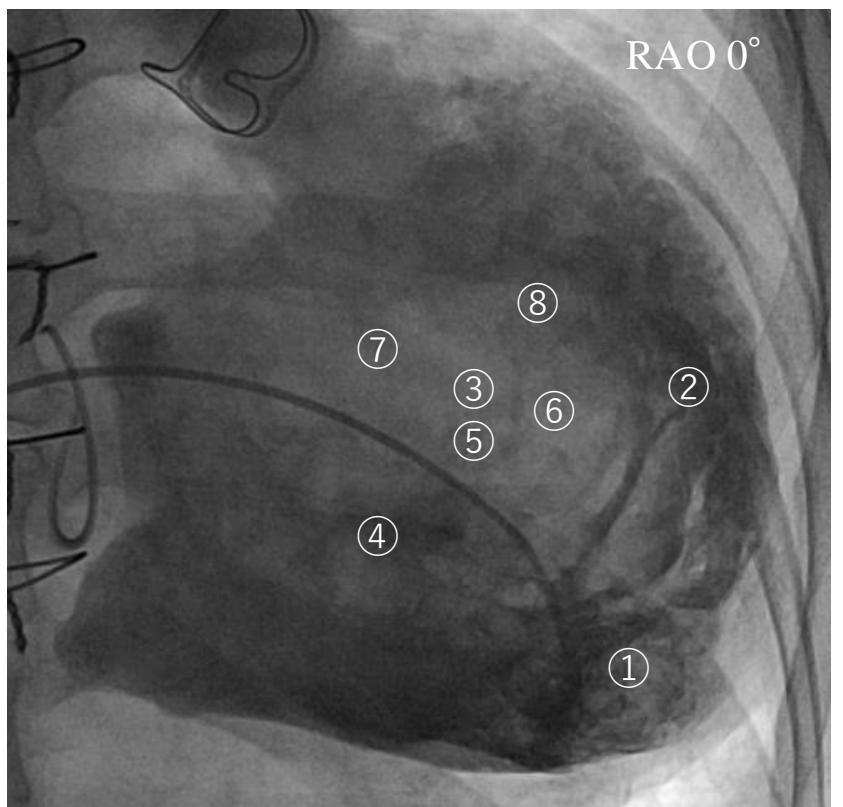

C

Pacing site No.	Pacing threshold @pulse width 1.0 msec	R wave sense	SICD vector		
			Primary	Secondary	Alternate
1	N/A	<b>1.34 mV</b>	X	O	X
2	N/A	<b>1.52 mV</b>	O	X	X
3	<b>3.0 V</b>	<b>2.19 mV</b>	X	X	O
4	<b>7.0 V</b>	<b>1.08 mV</b>	X	O	X
5	non capture	N/A			non capture
6	<b>7.0 V</b>	<b>2.18 mV</b>	X	X	O
7	non capture	N/A			non capture
8	<b>0.6 V</b>	<b>2.28 mV</b>	X	X	O

D

